

FastDryer User Guide

GVGT-2001

Version B

May 2014

GenTegra

1020 Serpentine Lane, Suite 110 — Pleasanton, CA 94566
ph 844-540-4000 — ph 925-461-3010 — fax 925-461-3086

support@GenTegra.com

WWW.GENTEGRA.COM

GenTegra

Summary

FastDryers are a simple and convenient way to dry biosamples following application to GenTegra-DNA (96- well microplates, racks of 0.3 ml cluster tubes, and 0.5 ml screw-cap tubes), GenTegra-RNA (0.5 ml screw-cap tubes and 0.3 ml cluster tubes), or GenPlates.

FastDryer Model GVGT2001

- Compatible with
- GenTegra DNA or RNA 0.5 ml screw-cap tubes ($\leq 50 \mu\text{l}$)
 - 96-well microplates ($\leq 250 \mu\text{l}$)
 - 0.3 ml cluster tubes, rack of 96 ($\leq 250 \mu\text{l}$)
 - GenPlates ($10 \mu\text{l}$)


- Specifications
- Dries 48 screw-cap tubes (0.5ml), one plate, or one rack at a time
 - Not for use with GenTegra-DNA 1.7 ml tubes

- Drying Time
- 16 hours

Cleaning the FastDryer

The FastDryer may be cleaned with mild soap and water and a microfiber cloth. RNaseZap or similar products may be used on the FastDryer. The use of bleach or ethanol is not recommended. The tube rack in the GVGT2001 is removable for cleaning.

GVGT2001 instructions

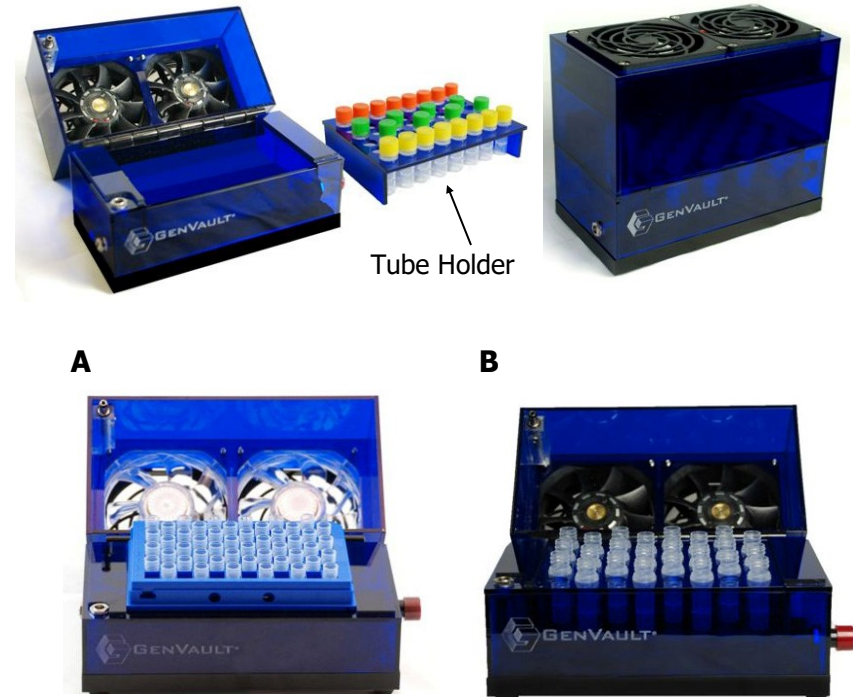

1. Before you begin: If you are using GenTegra DNA 0.5 ml screw cap tubes, refer to page 2, for volume requirements. Do not attempt to dry GenTegra DNA 1.7 ml tubes in the FastDryer.
2. Insert tube holder in FastDryer. Place rack of uncapped tubes, unsealed microplate or unsealed GenPlate on rack holder (A), or place up to 48 uncapped 0.5 ml screw-cap tubes in the tube holder (B).
3. Ensure that the power cord is plugged in and close the fan lid. Press the red ON/OFF switch to turn on the FastDryer.
4. Refer to page 2 for drying times.